

This Page Is Inserted by IFW Operations  
and is not a part of the Official Record

## **BEST AVAILABLE IMAGES**



Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

**IMAGES ARE BEST AVAILABLE COPY.**

**As rescanning documents *will not* correct images,  
please do not report the images to the  
Image Problem Mailbox.**

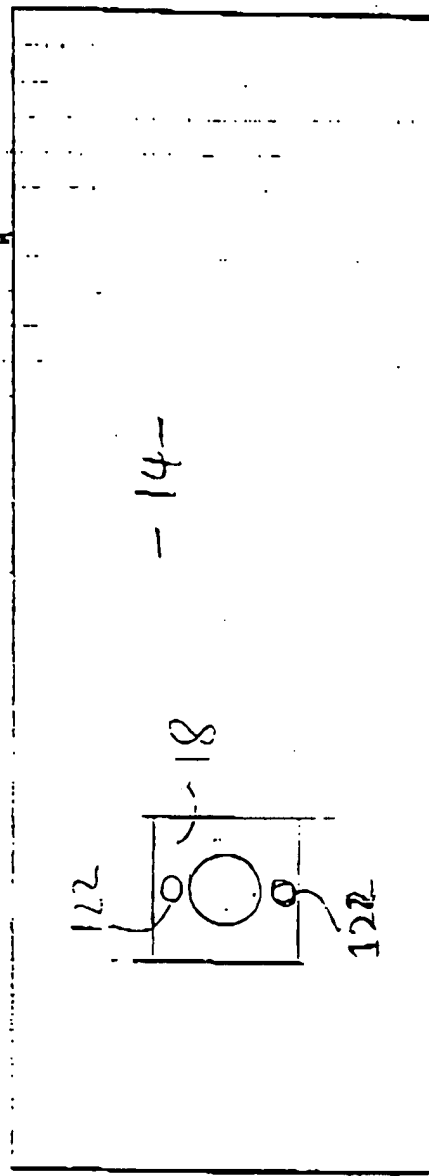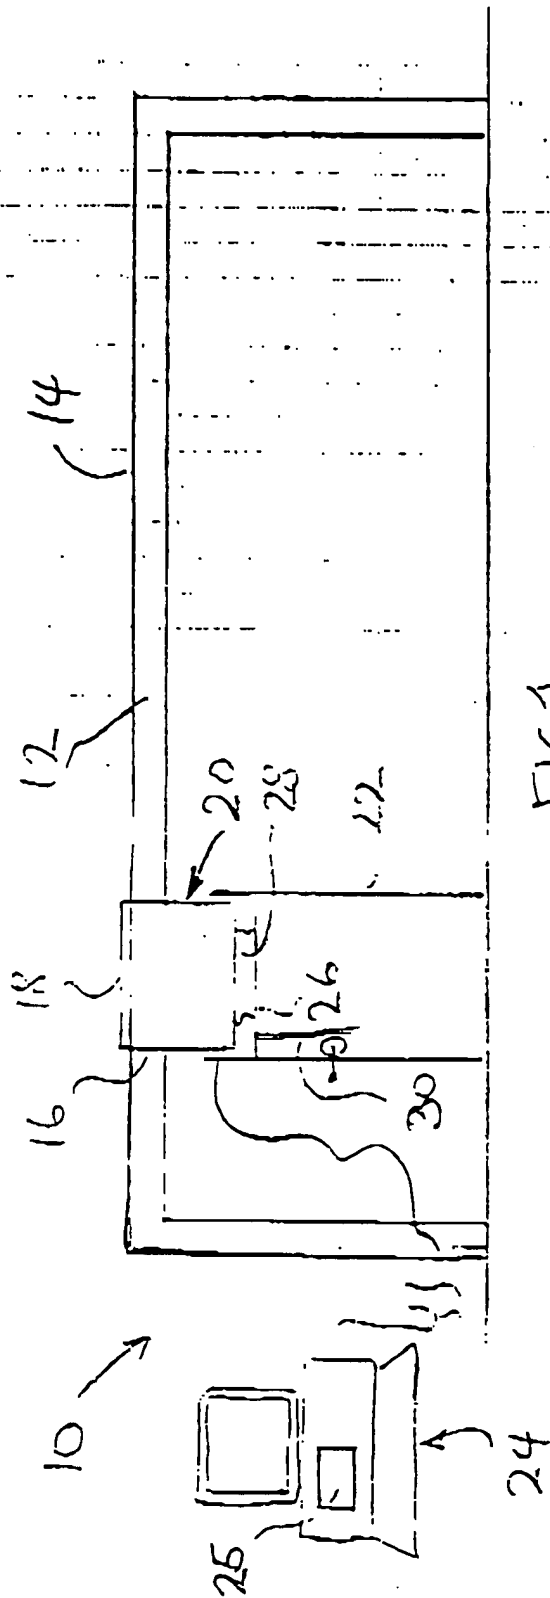

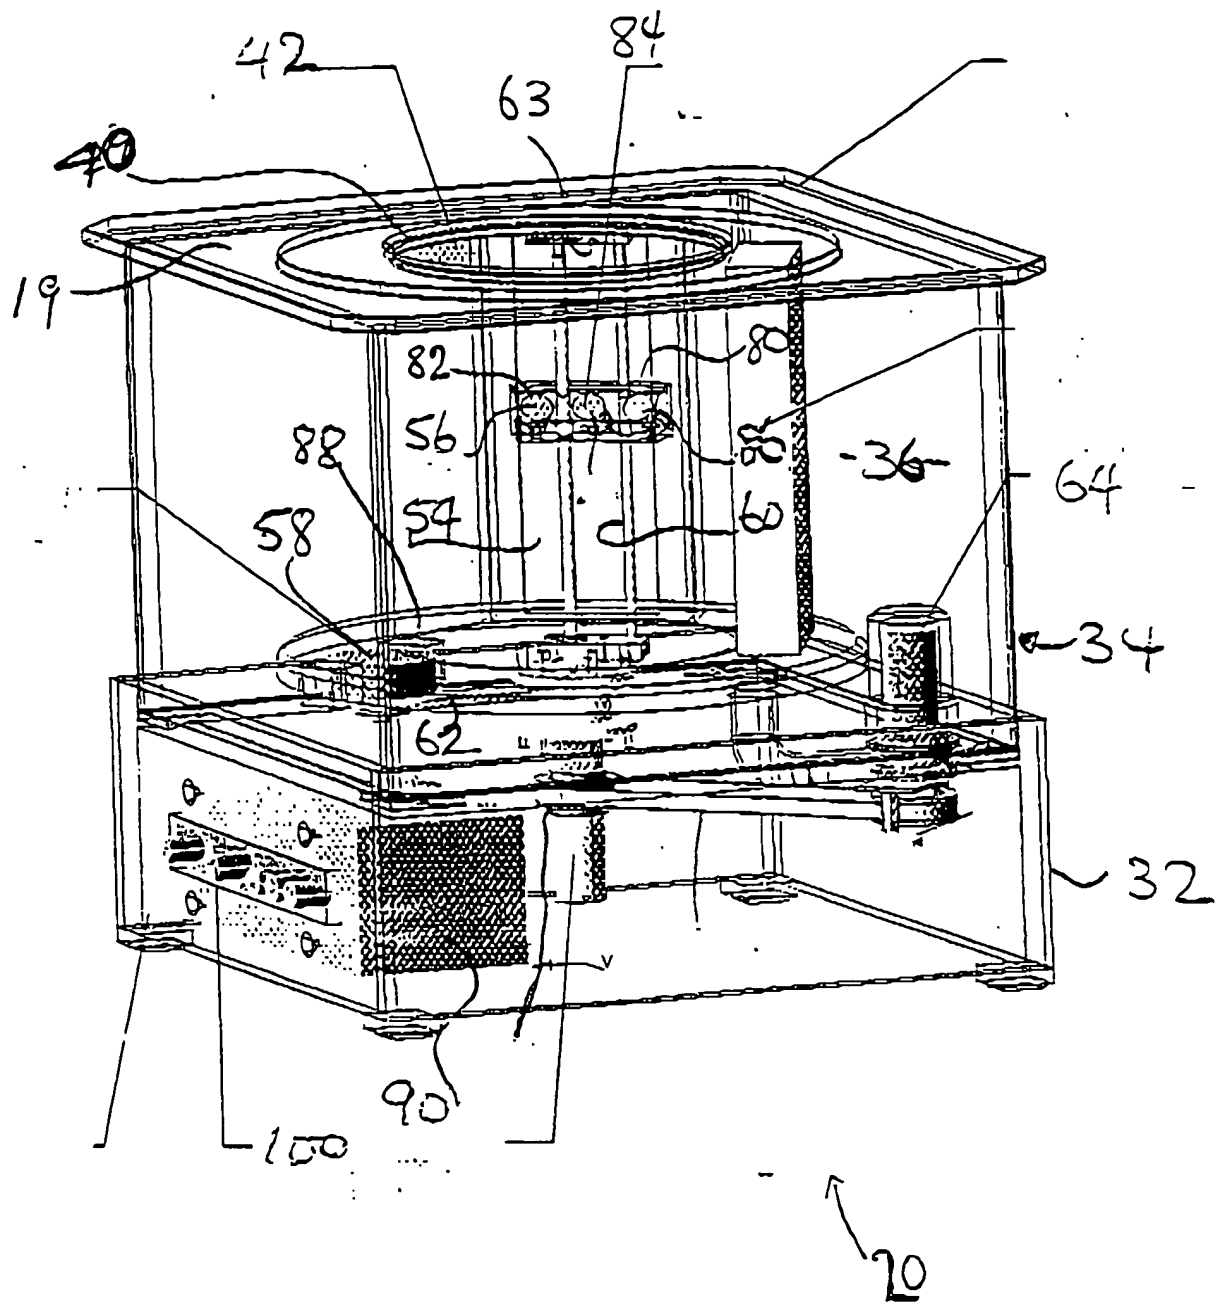


FIGURE 3

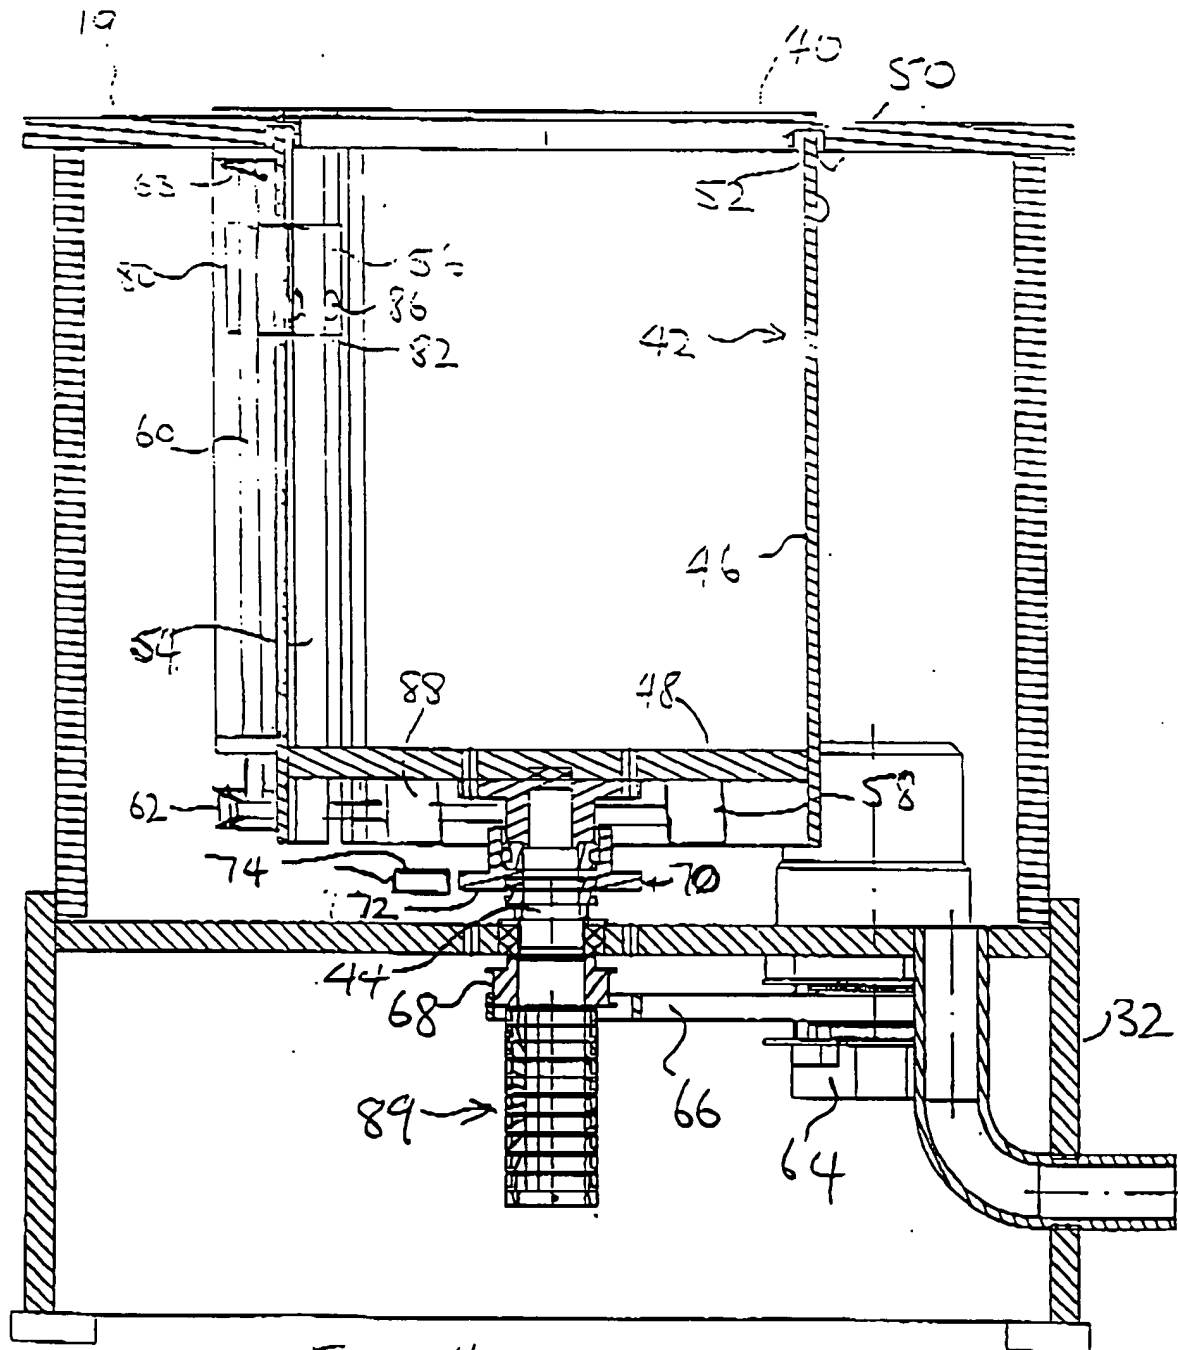
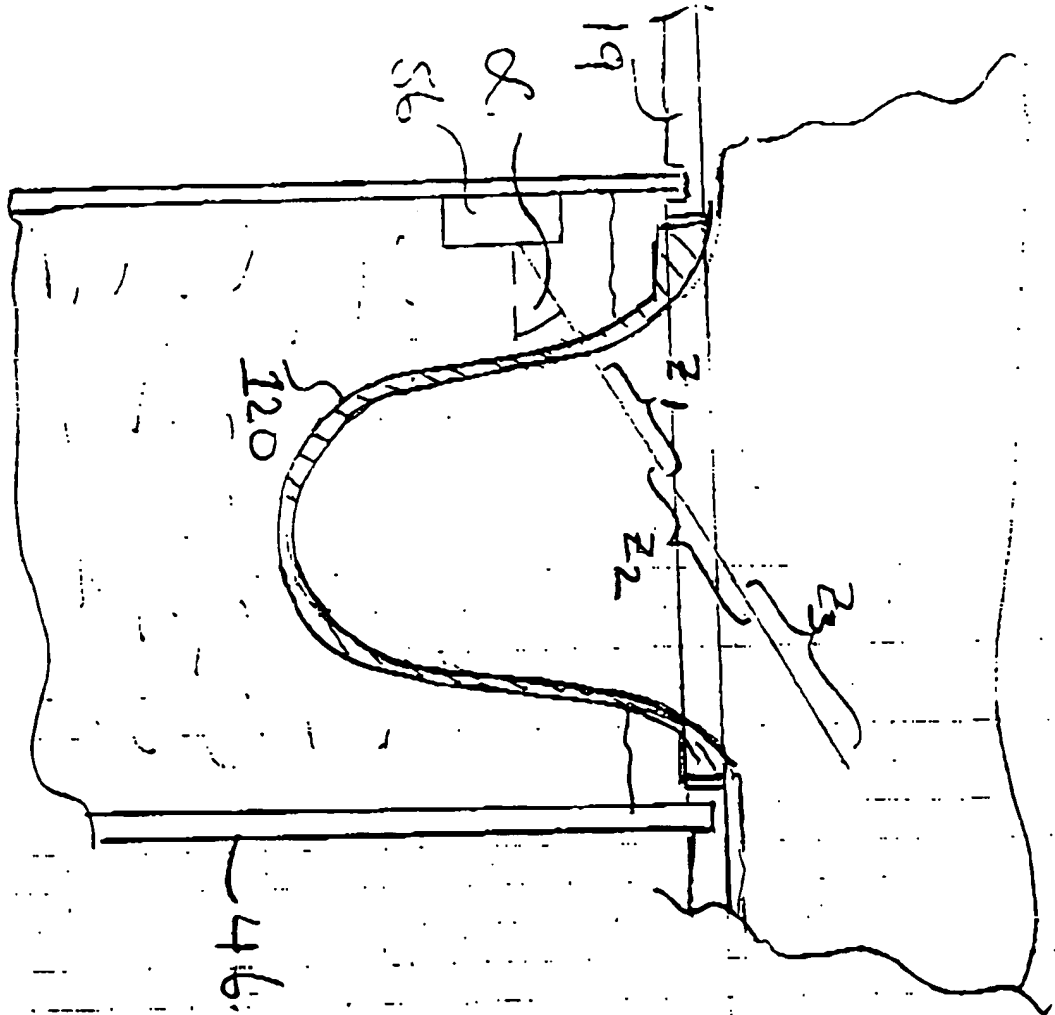


FIG. 4

FIG 5





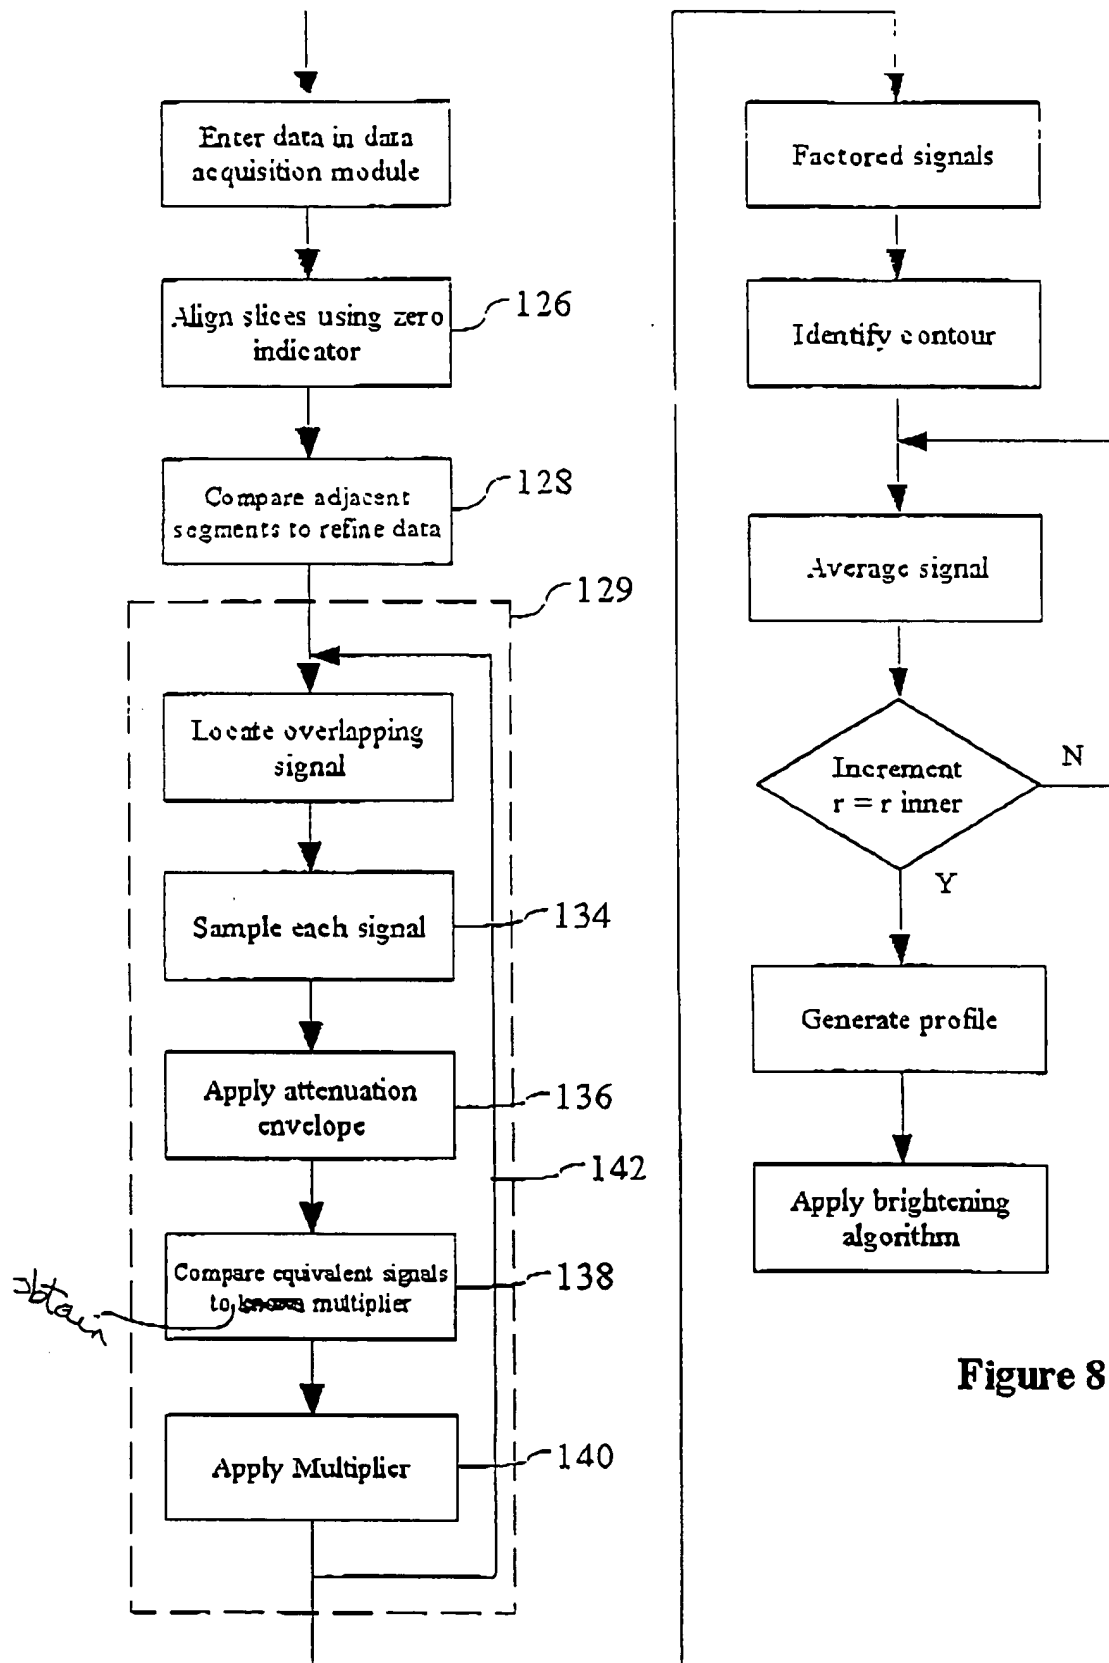


Figure 8

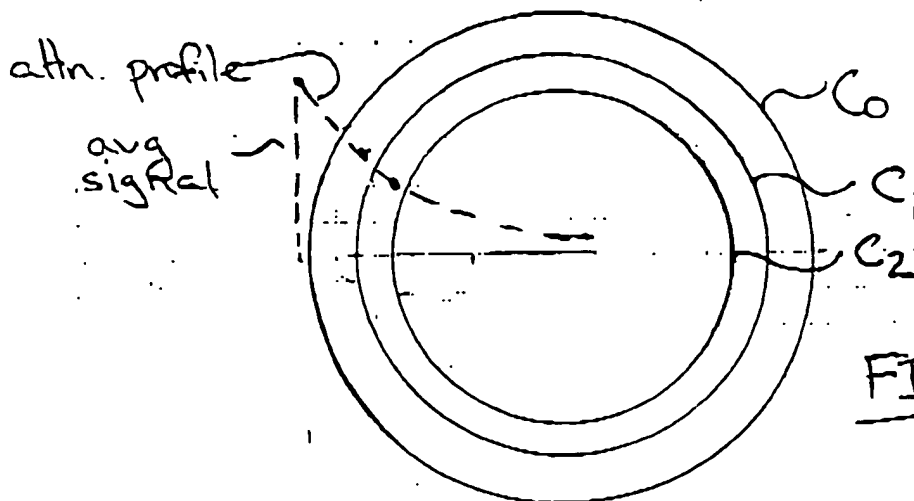
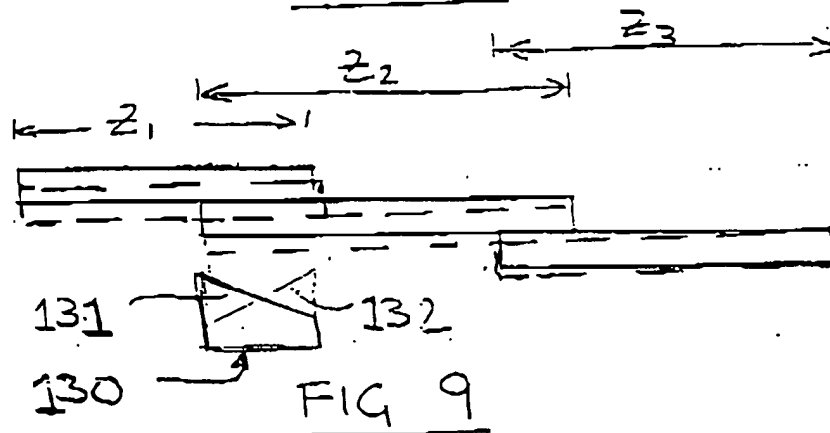
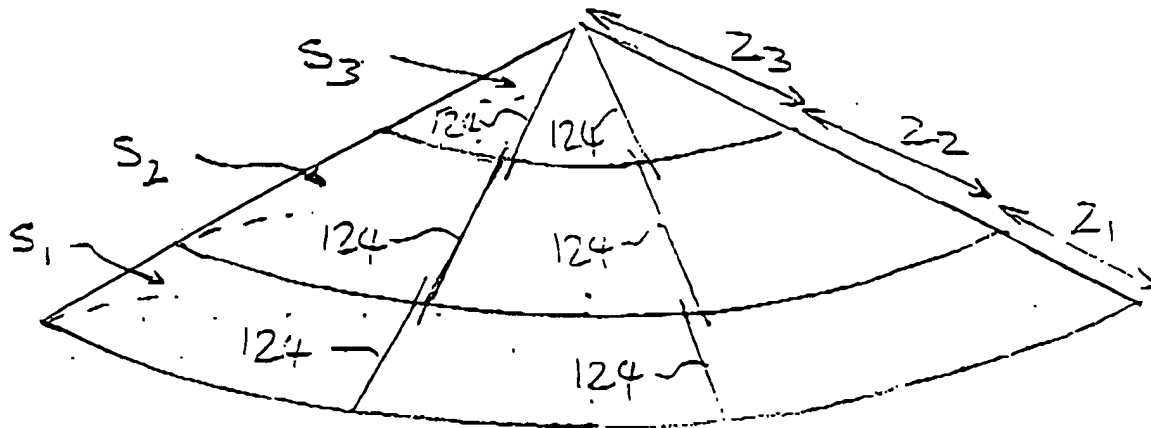




FIGURE 11

The Medipattern Corporation - Connected to MED

# medipattern

Registration Cabinet Scan MPR Logout

Acq. Params: **Region 1** **Area 1** **Serial 1**

USG USG Scanner 5

## Device Settings

Step Size (0.1mm): 10  
Vertical Count: 110  
Vertical Start (0.1mm): 0

## Card Settings

Amplifier: 1V/V  
Sampling: 20 MHz  
Breast: Right

Preview/Scan Mode: Quality Size: SizeB

## Transducer Preamp

17 25 31

## POWER

On Off GoTop

## VERTICAL MOTOR

<< UP DN >>

## Cine Controls

Cine Type: YoYo Loop  
Speed (0.5): 6  
Play Stop

Preview Scan RECON Key Display

## Acquisition

Folder ID: 1010 Name:

